

# Step-by-Step Guide to packing a Pilot Scale Glass Column

Packing of YMC PilotPLUS columns with soft gels



#### 1 Introduction

n this guide, all steps and relevant parameters for successfully packing pilot scale YMC PilotPLUS columns are presented.


When packing a glass column, different methods can be used. The selection of the most appropriate packing method depends on the column hardware, the packing material and the available system.

Apart from the selection of the resin, there are three consecutive steps which are relevant for column packing:

- 1 In the first step, the column, the system and the resin are prepared.
- The second step is the actual column packing.
- (3) The final step is the testing and qualification.

In this guide, the flow-packing method is described step by step for packing a pilot scale column. Flow packing is shown in the figure on page 3 in channel A. It consists of the consolidation and compression step during packing.

The three successive processes are shown as a flow diagram in the following figure:

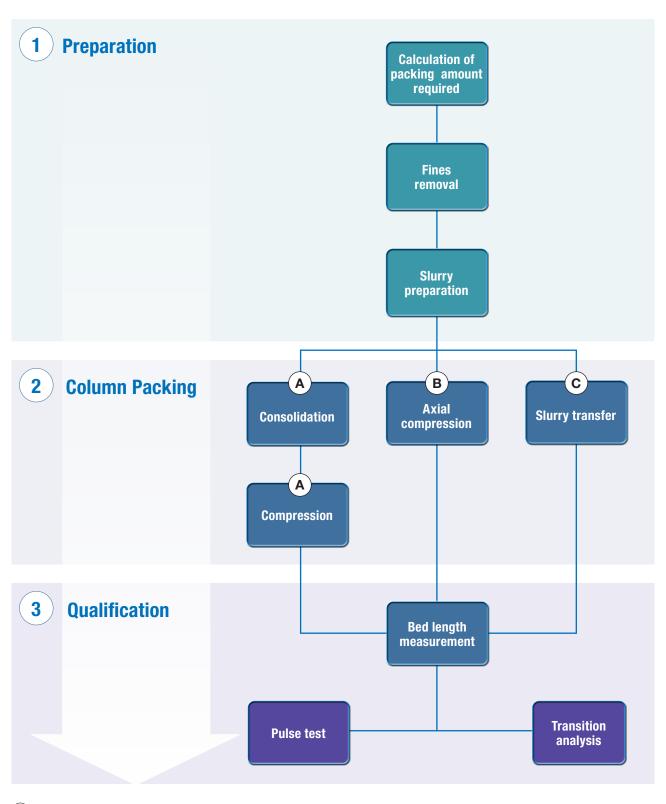


- (A) = Flow-packing
- (B) = Axial compression
- (c) = Qualification

All other terms are described on page 13.

#### What impact does the packing quality have on the chromatographic results?

The basis for every chromatographic separation is the correct choice of stationary phase. Only this way, can an optimum resolution be achieved. Of course, the packing material needs to be packed into the column as efficiently as possible for robust and reproducible results.



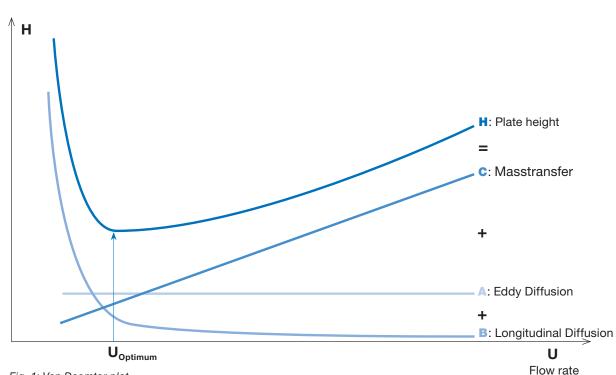


Fig. 1: Van Deemter plot

$$H = A + \frac{B}{u} + C \cdot u$$

$$A \quad B \quad C$$

Where

H = Plate height

A = Eddy Diffusion

B = Longitudinal Diffusion

C = Masstransfer

u = Flow rate

The A **term** represents the so-called Eddy Diffusion/spread diffusion effect. It describes the correlation between the plate height (H) and the particle diameter. The analytes take different paths through the column and this requires a different time. This results in peak broadening.

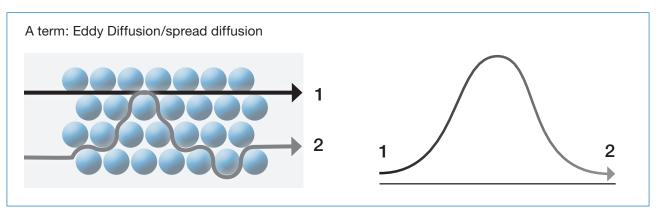


Fig. 2: Graphic description of the A term Eddy Diffusion

Through a homogenous column packing, the peak broadening is reduced. Therefore, the Eddy Diffusion is a direct measure for the packing quality of a column.

The **B term** describes the longitudinal diffusion. It depends on the viscosity and the temperature of the mobile phase. The B term becomes smaller for higher flow rates.

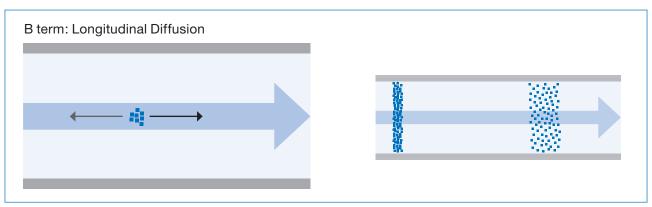


Fig. 3: Graphic description of the B term Longitudinal Diffusion

The **C** term describes the mass transfer of the analyte and therefore the establishment of the equilibrium between the mobile and the stationary phase. This term is affected by the porosity of the stationary phase and the column geometry.

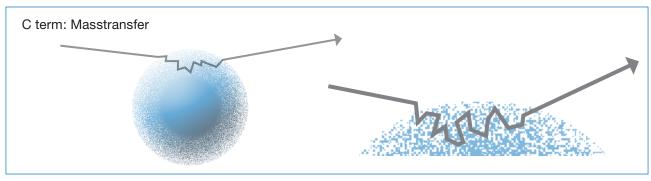


Fig. 3: Graphic description of the C term Mass Transfer

## 2 Preparation

# 2.1. Calculation of amount of packing required

1. Calculation of column bed volume:

$$V_{\text{bed}} = \frac{\pi \, d^2}{4} * l$$

2. Calculation of compressed gel volume:

$$V_{\text{material}} = V_{\text{bed}} * f_{\text{compression}}$$

- 3. Note the ratio of settled material and supernatant in the storage vessel.
- 4. Homogenise the material and the solvent in the storage vessel.
- Transfer the required amount of packing material to a graduated cylinder.
   Meet the ratio from step 3.

- 6. Let the material settle overnight.
- 7. Check the amount of settled material.

  If required, add or remove packing material.

#### 2.2. Removal of fines

1. Add four times the volume of solvent to the material.

Check the manufacturer's instructions for the selection of the correct solvent.

- 2. Homogenise the material and the solvent.
- 3. Decant the supernatant.
- 4. Repeat steps 1 to 3 until the supernatant is clear.

If required, add or remove packing material.

#### 2.3. Slurry preparation

- 1. Wash the packing material with at least three times the volume of packing solvent.
- 2. Collect the material in a beaker.
- Add sufficient packing solvent until you meet the required slurry concentration.
   You can wash the packing material inside the column.

# **Preparation**

Use the "YMC Glass and Pilot Column Packing Calculator"

!Do not use magnetic stirrers for homogenisation!

The duration of the sedimentation depends on the particle size: larger particles settle faster than smaller ones.

!Do not use magnetic stirrers for homogenisation!

!Do not let the soft gels dry out!

# **Preparation**

#### 2.4. System and column preparation

- 1. Flush the system for packing with the packing solvent.
- 2. Check the column parts with regards to cleanness and function.
- 3. Remove the adjustable end piece.
- 4. Connect the drainage tubing with the drain function. Place the drainage tubing in a collecting vessel.
- 5. Connect the pump to the tubing at the column body.
- 6. Start the pump.
- 7. Pump approx. 1–2 cm of liquid into the column from below.

  This way, air in the frits is removed.

  Take care that the liquid and the profile gasket are free of air bubbles.
- 8. Stop the pump and disconnect it from the column body.
- 9. Close the valve in the tubing of the column body.
- Adjust the vertical alignment of the column with a level.
   The adjustment of the column is important for a good packing result.
- 11. Connect the adjustable end piece (outside the column) with the pump.
- 12. Flush the adjustable end piece with liquid. This way, air is removed from the upper piston and frit.
- 13. Stop the pump and disconnect the adjustable end piece from the pump.

#### 3 Packing

 Place the infilling assistance on top of the column.



- 2. Connect the drainage tubing with the drain function. Place the drainage tubing in a collecting vessel.
- 3. Homogenise the slurry.

Stir constantly in one direction in order to avoid the entry of air.

A mixing duration of 5 minutes is common.

For air removal, the slurry can be put in an ultrasonic for 5 minutes. Afterwards, the slurry needs to be homogenised again.

- 4. Pour the homogenised slurry quickly through the infilling assistance in the open column. If no infilling assistance is used, pour the slurry down the opposite side of the glass wall in order to avoid the entry of air.
- When the material is completely transferred into the column, clean the glass wall with packing solvent to remove any remaining particles.

Only in this way can optimum sealing of the profile gasket be guaranteed.

- 6. Fill the column completely with packing solvent until it reaches the upper edge of the drain function
- Turn the closing disc of the adjustable end piece in UP direction as far as it will go. Afterwards, turn the closing disc half turn in DOWN direction.

The adjustable end piece is ready for insertion into the column body.

# **Packing**

Avoid the entry of air.

Carry out steps 2–15 as quickly as possible in order to avoid resettlement of the material.

Very important for columns with permanent sealing.

# **Packing**

 Put the adjustable end piece in a slight angle opposite the drain function on the colum body.



- 9. Bring the piston slowly into a vertical position. This way it ensures that no air is trapped below the frit.
  - Excessive slurry solvent will flow into a reservoir through the drainage tubing.
- 10. Screw in the star screws and close the column this way.
- 11. Lower the adjustable end piece until it is filled completely with liquid.

  Liquid comes out of the upper piston.
- 12. Remove the air from the tubing.
- 13. Connect the pump to the tubing of the adjustable end piece.
- 14. Open the valve in the tubing of the column body.
  - The lower tubing can be put into the storage vessel of the packing solvent. This way the packing solvent can be recycled.
- 15. Increase the flow rate stepwise until you reach the required flow rate and packing pressure.

  Wait after every step until the pressure is con stant and only increase the flow rate once the pressure has stabilised.
- 16. Wait until the column bed has formed and the bed length does not change anymore. For checking, mark the bed length under flow.
- 17. Decrease the flow rate stepwise until the pump can be stopped.
- 18. Close the valve in the tubing of the column body.

# **Packing**

- 19. Disconnect the pump from the adjustable end piece.
- Lower the upper piston until you reach the column bed.

Take care that the upper piston is filled with packing solvent completely and that liquid comeas out.

- 21. Remove the air in the tubing of the system.
- 22. Connect the adjustable end piece to the pump.
- 23. Open the valve in the tubing of the column body.
- 24. Increase the flow rate stepwise until you reach the required flow rate and packing pressure.
- 25. Wait until the bed length does not change anymore.

If the packed bed compresses further, mark the new position of the bed under flow. Continue with steps 26–34.

If the packed bed does not compress further, continue with steps 26–28 and then step 35.

- 26. Decrease the flow rate stepwise until you can stop the pump.
- 27. Close the valve in the tubing of the column body.
- 28. Disconnect the pump from the adjustable end piece.
- 29. Lower the adjustable end piece until you reach the column bed.

Take care that the upper piston is completely filled with liquid and solvent comes out.

- 30. Remove the air from the tubing of the system.
- 31. Connect the pump to the adjustable end piece.
- 32. Open the valve in the tubing of the column body.
- 33. Increase the flow rate stepwise until you reach the required flow rate and packing pressure.
- 34. Go back to step 25.
- 35. Lower the adjustable end piece until you reach the last mark (mark under flow).
- 36. The column is now finally packed.
- 37. Connect the column to the system for testing and qualification.

## 4 Testing and qualification

- 1. Measure the bed length.
- Equilibrate the column with 5 column volumes of the recommended qualification solvent.
   Check the product instructions from the packing material supplier.
   The flow rate is the same as the flow rate for qualification.
- 3. Perfom the qualification corresponding to the manufacturer's recommendations or guidelines.
- 4. Repeat the quality control 3 times. This way, the reproducibility of the results is obtained.
- 5. Evaluate the column packing and qualification.

  If the required specifications are met, the column is now ready for use.

  If the required specifications are not met, return the column and the system to the packing solvent, unpack the column and repeat the packing process.

## Qualification

### 5 Unpacking

The column will require unpacking if the required specifications are not met in the qualification run or if the material has to be changed or replaced.

- 1. Put a collecting vessel below the column stand.
- 2. Close the column at the column body.
- 3. Remove the adjustable end piece from the column.
- 4. Loosen the locking bolts at the column stand.
- 5. Lift the column body from the column stand.
- 6. Put the column body into the stand with the open end facing the locking bolts.



- 7. Connect the system to the column body.
- 8. Increase the flow rate stepwise.

  The packing material is pressed out of the column.
- 9. As soon as all the material is in the collecting vessel, stop the pump.
- 10. Clean the column for the next packing or storage.
- 11. Prepare the material as described by the manufacturer's instructions for re-packing or storage.

# **Unpacking**



#### **Terms and definitions**

**Axial compression** The material is compressed in a one-step process by lowering the piston

onto the column bed. The piston movement stops at a defined pressure.

**Compressibility** Soft gels are compressible due to their polymeric base particle.

This need to be considered when column packing.

Compression The consolidated bed is compressed under flow or manually in order to

receive the final column packing.

**Consolidation** First step in flow packing in which a loose column bed is formed.

**Fines** Broken particles which float on the liquid surface of the slurry.

These need to be removed from the slurry in order to receive a

homogenously packed column bed.

**Pulse test** Evaluation of the detector signal after injection of a defined substance.

Slurry Suspension of packing/slurry solvent and packing material.

**Slurry concentration** Concentration of the packing material in the packing/slurry solvent.

Most often, this is a concentration range which is mentioned in the

instructions from the packing material supplier.

Slurry transfer Also known as Pack-In-Place. The piston is already adjusted.

The slurry is pumped into the column until a defined pressure is reached.

**Transition analysis** Evaluation of the detector signal of a gradient.

**Unpacking** Removal of the packing material from the column.



